

**RESEARCH ARTICLE**

# Anthropometric Measurements of Distal Femur to Design the Femoral Component of Total Knee Arthroplasty for the Iranian Population

Ali Birjandinejad, MD<sup>1</sup>; Reza Zandi, MD<sup>2</sup>; Elham Karimi, MSc<sup>3</sup>

*Research performed at Imam Reza Hospital in Mashhad, Iran*

*Received: 07 June 2018*

*Accepted: 08 December 2018*

**Abstract**

**Background:** Acquiring knowledge about anatomic and geometric quantities of bones is among the most vital parameters in orthopedic surgery that has a significant effect on the treatment of various disorders and subsequent outcomes. The aim of this study was to obtain anthropometric information for distal femur in order to compare with similar dimensions of prosthesis used in total knee arthroplasty (TKA) surgery and to design more suitable and optimal components.

**Methods:** Morphological data of distal femur were measured in 132 knees (81 males and 51 females) using magnetic resonance imaging (MRI). The data included anterior-posterior (AP) length, medial-lateral (ML) width, medial AP (MAP), lateral AP (LAP), MAP to LAP distance in the anterior distal femur namely anterior medial lateral (AML) width, medial and lateral condyle width, and intercondylar notch. The aspect ratio (ML/AP) was also calculated and the results were compared with similar dimensions of currently used knee implants.

**Results:** Our data showed that men are significantly larger in all dimensions than women. In the distal femur with similar AP lengths in both sexes, women had a smaller ML width than men ( $P < 0.001$ ). Comparison between the distal femur and studied prostheses showed no high correlation and similarity between the femoral component and femoral condyle prostheses in the resected surface of the bone.

**Conclusion:** The results of this study can provide the data needed to design prostheses suitable for the Iranian population.

**Level of evidence:** III

**Keywords:** Anthropometric, Distal femur, Knee, Magnetic resonance imaging, Prosthesis

**Introduction**

Knee joint is the largest weight bearing and transferring joint in the body. It is subsequently affected by various inflammatory and degenerative diseases, ultimately destroying the articular cartilage and proper joint function. Symptoms of knee joint disorders are characterized by pain, joint instability, reduced range of motion, and deformity (1).

There are different therapeutic approaches for solving this problem including changing the lifestyle, weight loss, nonsteroidal anti-inflammatory drugs (NSAIDs), physiotherapy, muscle strengthening, use of a cane, use of brace, and debridement and osteotomy, all of which are palliative methods that only reduce pain and delay the course of the disease. The disease progression

**Corresponding Author:** Elham Karimi, Department of Biology and Anatomical Sciences, Faculty of Medicine, Shahid Beheshti University of Medical Sciences, Tehran, Iran  
Email: elham.karimi@sbmu.ac.ir



THE ONLINE VERSION OF THIS ARTICLE  
ABJS.MUMS.AC.IR

leads to the need for definitive and final treatment of the disease, which is the total knee arthroplasty (TKA) surgery (1-6).

Although TKA has been associated with many successes, it has some disadvantages; for example, prosthetic damage results in a revision surgery that imposes a much higher cost and more dangers. For this purpose researchers have always sought to find ways to increase the longevity and durability of prosthesis, one of which is the design of prosthesis that are appropriate to the anthropometry of each population as the success rate of TKA largely depends on the choice of prosthesis, the exact size, and the correct location of its components. Adherence to these principles is very important in the success and long-term survival of TKA prosthesis (7-9).

In this study, we decided to measure the anthropometric dimensions of distal femur and compare with available prostheses, as well as examining the necessity of gender-specific prostheses.

### Materials and Methods

This descriptive study was performed on 132 knees using MRI at Imam Reza Hospital, Mashhad, Iran, in 2015.

Informed consent was obtained from all participants in this study. The proposed study was approved by the ethics committee of Shahid Beheshti University of Medical Sciences.

The inclusion criteria were age between 20 to 60 years and normal lower extremity alignment. Patients with advanced arthritis history and any rheumatoid conditions, previous fractures in distal femur, osteophytes and gross congenital anatomy or deformity

were excluded from the study.

The individual femur contour following each resection was exported for further analysis. All MRIs were analyzed by pmsD view (Philips DICOM Viewer, R3.0 SP3, 2013) program.

### Measurement of distal femur

To simulate femoral bone with a TKA surgical incision, a line was drawn in the frontal plate at 10 mm above the articular level, followed by measuring the anterior-posterior (AP) length, medial-lateral (ML) width, medial AP (MAP) length, lateral AP (LAP) length, and anterior medial lateral (AML) width in the axial plan. The width of the medial and lateral condyles (WM, WL) and intercondylar notch (WI) were also measured [Figure 1]. All measurements were recorded in millimeters. To measure the AP length, a line was drawn from the anterior cortex, the posterior femoral AP was also obtained by a line drawn as described by Ho et al. (10), according to this method:

The measured points were 10mm on the medial condyle and 8mm on the lateral condyle from the lowest points on the medial and lateral posterior condyles.

MAP and LAP are the longest lines drawn in femoral medial and lateral compartments, respectively. AML is the distance between the two MAP and LAP points in the anterior distal femur. The sum of the medial and lateral condyle widths and the inter-condylar notch represent the ML width [Figure 1].

Additionally, the aspect ratio (the ML dimension divided by the AP dimension  $\times 100$ ) was calculated as well. The measured dimensions were compared with four available femoral components, including NexGen,

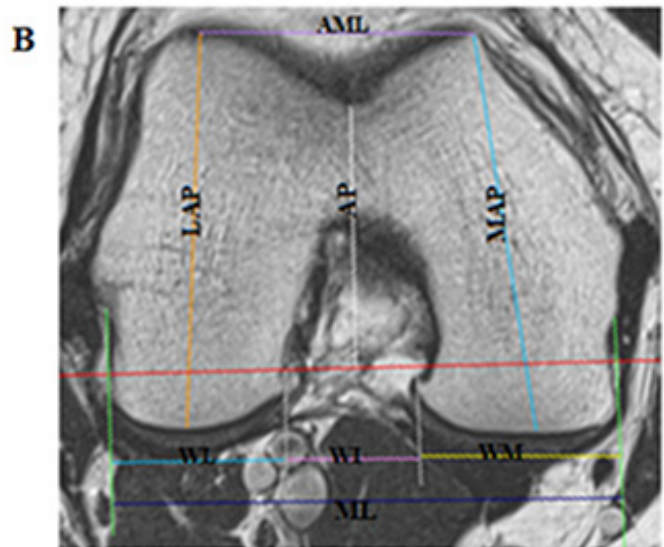
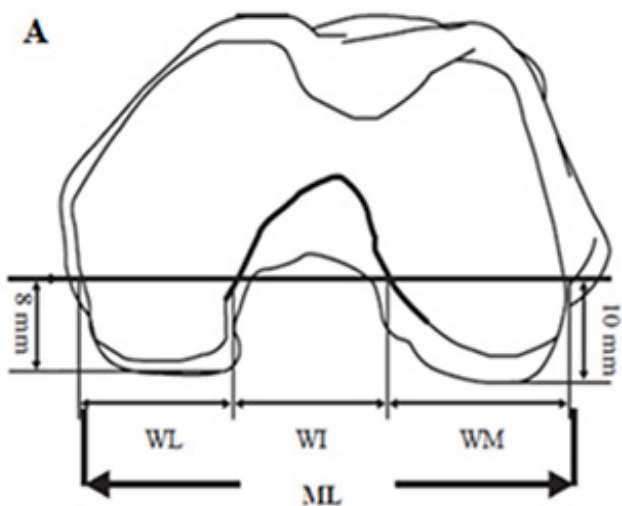


Figure 1. Schematic representation(A)(10) and Axial MRI image(B) of the distal femur resected surface, showing the measurement methods used in the MR analysis.

MAP and LAP are respectively medial anterior-posterior length and lateral anterior-posterior length; AML is medial lateral width in anterior distal femur. WL, WM and WI are the width of lateral condyle, medial condyle and intercondylar notch respectively.

Scorpio, GenesisII and Aesculap, and a gender-specific femoral component (NexGen-csf prosthesis). The ML and AP values and ML/AP aspect ratio were also calculated for the prostheses.

### Statistical analysis

SPSS version 22 software was used for statistical analysis. Descriptive statistics were used to measure the variables. For comparison between men and women, the student t-test was used for parametric variables, and the Mann -Whitney test was used for nonparametric variables. Finally, linear regression was used to compare the results and determine the cut correlation of simulated bones with the dimensions of the prostheses. *P value* <0.05 indicated a significant difference.

### Results

A total of 132 patients, including 81 men (62%) and 51 women (38%) aged 20-60 years, were enrolled in the study.

The mean AP length was 42.22±4.89 mm; the mean ML width was 67.53±6.66 mm; the mean WM, WI, and WL were 26.72±3.41 mm, 20.90±3.31 mm, and 24.49 ± 2.49 mm; the mean MAP was 53.88±6.64 mm; the mean LAP was 55.85±5.44 mm; the mean AML was 37.75±4.74 mm; and the mean ML / AL aspect ratio was 1.61±0.16.

Regarding the distal femoral morphology, our data showed that, except for LAP/ML in all dimensions, men were significantly larger in size than women (*P*<0.05), MAP/ML and MAP/LAP variables were not significantly different (*P*>0.05) between men and women [Table 1].

### Comparison of distal femur dimensions with available prostheses

Comparison between the distal femur and prostheses (NexGen, Scorpio, GenesisII, and Aesculap) showed a low correlation between all femoral component prostheses and femoral condyle in the resected surface of the bone [Figure 2].

In this study, we compared the mean AP and ML dimensions with gender-specific prosthesis (NexGen). For further investigation, the distal femur morphology was examined separately among the sexes [Figure 2]. It was found that the mean AP and ML dimensions in the female knee were more fit with gender-specific prostheses. Simply put, in the Iranian population, like other ethnic groups, women have a smaller ML size for a similar amount of AP that justifies the use of gender-specific prostheses. As shown in various studies, there are differences between men and women in modern total knee arthroplasty [11-14].

In terms of prosthetic fitting among the sexes, all prostheses indicated size mismatch in larger and smaller sizes. In women, the implants tended to undersize in smaller AP dimensions and overhang in larger AP dimensions. In men, almost all prostheses in the ML dimensions tended to undersize with an increase in AP dimensions [Figure 2].

In the comparison graphs of the aspect ratio, a different trend can be seen between men and women [Figure 3]. An increase in AP size, the ML/AP aspect ratio indicated a gradual decrease in men and a mild upward in women.

The femur aspect ratio on data simulated in men showed a greater ratio for smaller knees and a lower ratio for larger knees.

Table 1. Anthropometric Measurements of distal femur resected surface

Parameters	Male	Female	Total	<i>P-value</i>
Age(year)	35.12±11.75	43.59±10.23	38.39±11.89	<0.001
Dimension(mm)				
ML	71.31±5.22	61.53±3.55	67.53±6.66	<0.001
AP	43.80±4.34	39.72±4.69	42.22±4.89	<0.001
MAP	56.18±6.14	50.24±5.77	53.88±6.64	<0.001
LAP	57.91±4.90	52.57±4.63	55.85±5.44	<0.001
AML	39.98±4.06	34.22±3.43	37.75±4.74	<0.001
WI	22.37±2.82	18.58±2.65	20.90±3.31	<0.001
WM	28.22±2.82	24.33±2.89	26.72±3.41	<0.001
WL	25.58±2.17	22.76±1.94	24.49±2.49	<0.001
Aspect ratio				
MAP/ML	0.79±0.08	0.82±0.07	0.80±0.08	0.056
LAP/ML	0.81±0.07	0.85±0.07	0.83±0.07	0.001
MAP/LAP	0.97±0.05	0.95±0.06	0.96±0.06	0.143
ML/AP	1.64±0.15	1.56±0.16	1.61±0.16	0.008

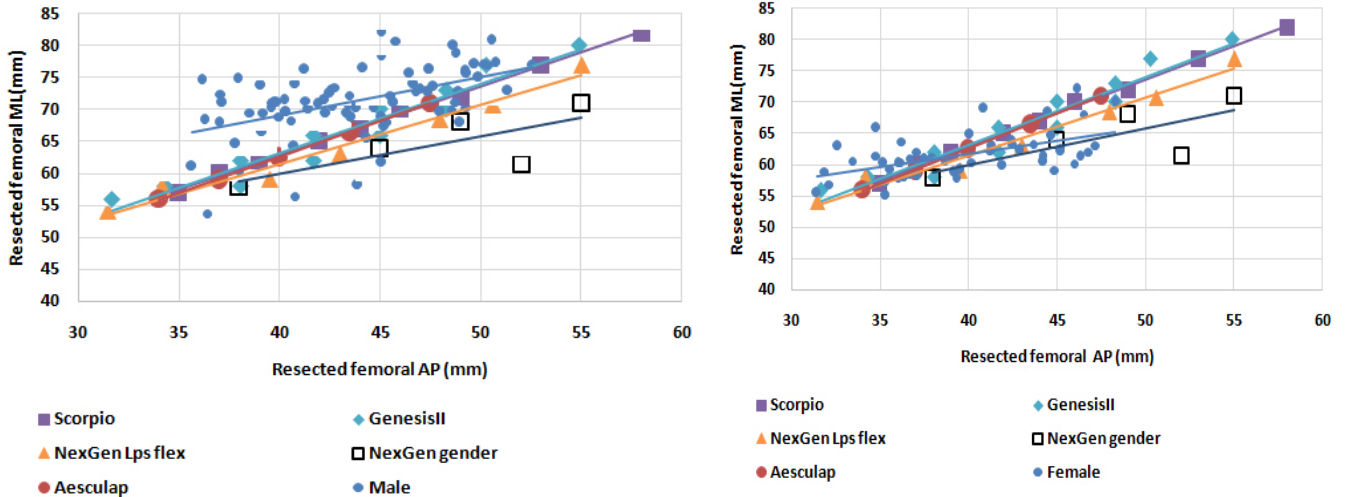


Figure 2. The relationship between the ML and AP dimensions of the examined population with the femoral components available in men and women.

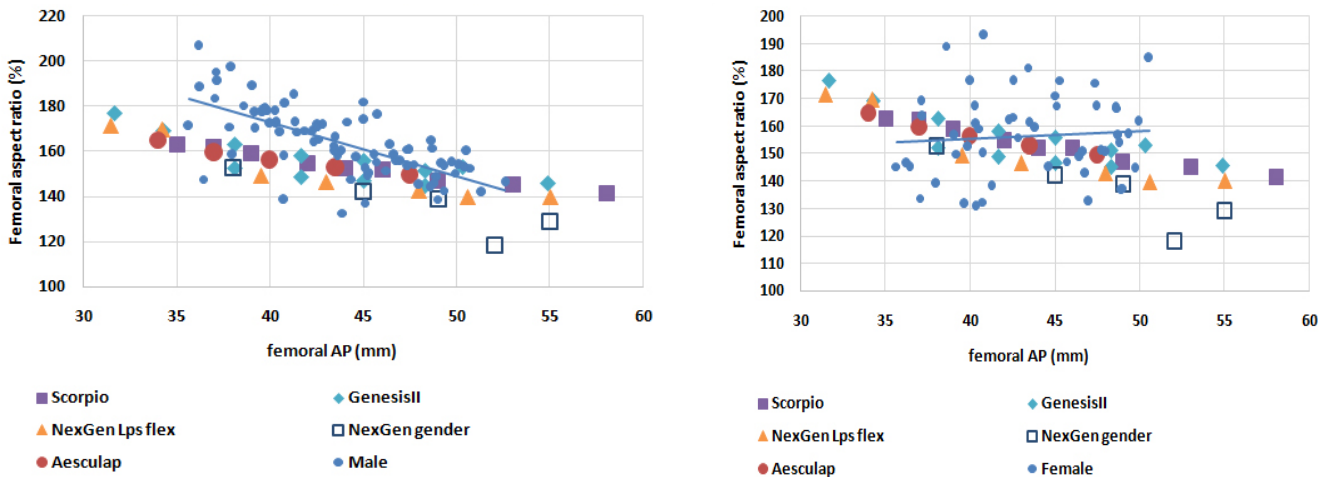


Figure 3. The relationship between the AP/ aspect ratio of the examined population with the femoral components available in men and women.

### Discussion

Modern total knee arthroplasty began with the development of condylar knee prosthesis in 1970 and is considered one of the most successful orthopedic surgeries, according to the knee association. The main indication of knee joint replacement is the removal of severe knee pain with or without deformity (15, 16).

As noted in the literature, in addition to the patient's condition and surgical procedure, improving the design of the prosthesis promotes the normal functioning of patients after TKA surgery (17).

It is well-known that the Asian population has smaller dimensions of the knee than its western counterparts and imported implants, which are mainly based on Western anthropometrics, are unsuitable for patients in Asian countries (18-20). Therefore, anthropometric

and morphological studies of different ethnic groups are required to improve the quality, shelf-life, and longevity of prostheses.

Our study on the same distal femur AP size in both genders showed that women had a smaller medial-lateral size than males ( $P < 0.001$ ), similar to those of the study in Korea (21). There was also a significant difference in the resected surface between the sexes and the measured parameters; in all of these parameters, the amount in men was higher than that of women. Mahfouz et al. in the Caucasus showed that the anterior condylar height and eminence in women are less than that of men (22). Dargel et al. reported significant differences between male and female samples, as the knee dimensions in men in many parameters were significantly higher than women (23).

**Table 2. Comparison of findings from distal femur in different countries**

		Thai <sup>26</sup> (Chaichankul) (Resected)	Korean <sup>21</sup> (By Lim) (Non resected medial&lateral condyles)	Malay <sup>25</sup> (By Hussain) (Non resected)	Iranian <sup>27</sup> (By Moghtadaei) (Resected))	Iranian (our study) (Resected)	Chinese <sup>18</sup> (By Yue) (Non resected)	Chinese <sup>20</sup> (By Cheng) (Resected)	White's <sup>18</sup> (Non resected)
<b>AP</b>	Total	45.43± 4.5	59.6&58.7		44.9±4.1	42.22±4.89		64.1±2.7	
<b>Length (mm)</b>	Male	48.55±3.73	62.7&59	63.93±3.39	46.87±3.3	43.80±4.34	65.0±2.8	66.6±2.4	67.5±3.6
	Female	43.32±3.69	56.8&58.4	57.39±3.29	41.55±3.1	39.72±4.69	58.8±2.5	61.0±2.7	59.7±2.6
<b>ML</b>	Total	64.06±6.31	78.6±5.1		67.06±6.39	67.53±6.66		71.0±3.0	
<b>Width (mm)</b>	Male	70.15±3.87	81.5±5.7	74.88±3.55	70.71±4.1	71.31±5.22	82.6±3.6	74.4±2.9	86.0±5.6
	Female	59.91±3.75	76.7±3.7	64.53±3.12	60.56±4.2	61.53±3.55	72.8±2.6	66.8±3.1	76.4±4.0
<b>Aspect ratio (ML/AP)</b>	Total	1.41±1.2	1.31&1.25		1.49±0.11	1.61±0.16		111.1±2.7	
	Male	1.45±1.1	1.17&1.18	1.17±0.05	1.51±0.11	1.64±0.15	1.27±0.03	111.7±3.3	1.28±0.07
	Female	1.39±1.2	1.33&1.32	1.13±0.05	1.46±0.1	1.56±0.16	1.24±0.04	109.6±3.6	1.28±0.06

Comparison of distal femur dimensions in Table 2 shows racial differences that may be important for the design of implants.

We measured the ML width for further fitting with TKA surgical incision in the condylar surface; Studies conducted in India, Korea, China and Malaysia on anatomical intercondylar axis, other studies in Table 2, like ours, computed the ML width in the condylar surface, which makes the reported results smaller (19, 21, 24, 25). However, we are unable to compare our population and dimensions with other studies in this area because of the differences in imaging and measuring techniques (20, 26, 27).

In examining the measured dimensions of knee bones, it was found that there are different ML widths for a constant AP value. In contrast, most implant systems consider only one ML width for an AP length [Figure 2] Therefore, implants with multiple ML widths should be designed for an AP length to get better anatomical fit. The need for gender-specific prosthesis in knee joint replacement surgery is a part involved in the recent orthopedic community.

Clinical trials done so far, regardless of the patient's gender, have proven that TKA surgery successfully eliminates pain in patients with knee osteoarthritis and improves knee function (28-34). However, orthopedic surgeons accept the differences in knee anatomy between men and women. Numerous studies support the existence of such gender changes but, the clinical relevance of these differences is still unclear (11-13, 28, 35, 36).

Conley et al. argued that since the mean female distal femur is more trapezoidal, when using standard prostheses with respect to gender differences in the size of medial condyle and lateral distal femur, female patients may receive too many large patello-femoral

components (12). In the main dimension in femoral component implant, the AP length and ML width are used to select the appropriate size for each patient. The AP length is widely utilized as the main parameter for the implant size, as, it is strongly associated with the moving and walking and symmetric balanced flexion and extension gaps (37).

It is also very important to understand the relationship between the AP length and the ML width of the knee joint for implant design.

Chin et al. suggested that when the size of a prosthesis is determined based on the AP length, if the ML width of the prosthesis is larger than the ML width of the resected distal femur surface, it will lead to ML overhang, which may lead to soft tissue inflammation and imbalance (14). Other studies have also shown that in the distal femur with the same AP length in both genders, women have a smaller ML width. Therefore, if the implant components are made according to the femoral AP length, the ML width may overhang (11-13, 35).

Wei-pin et al. compared AP and ML dimensions of the subjects with the Uknee, NexGen, and Duracon systems and found that in a similar AP length, the ML width in these prostheses was greater than the ML width in the resected surface of the bone. Therefore, this implant tended to the ML width overhang in the distal femur resected surface in Chinese patients. In this study, the aspect ratio for femur bone in the resected surface of the bone showed a higher ratio for smaller knees and a lower ratio for larger knees, but, the examined prostheses showed slight changes in the aspect ratio compared to the AP length (10).

#### **Study limitations**

1. We did not calculate the two variables of height and weight of patients as independent factors in the distal

femur dimensions.

2. Our samples were young and healthy knees, which may be unsuitable for people with degenerative arthritis who are candidates for TKA surgery.

3. Statistical homogenization was performed for age; however, the results might be affected due to the age difference between male and female samples.

4. Due to the large diversity in ethnicity in Iran as well as the importance of morphological and anthropometric indices of tibial and femoral bones, it is recommended that similar researches should be carried out more widely and in other parts with larger statistical sample sizes.

A wide range of two measured ML and AP dimensions has been distributed excessively in this study. Therefore, an implant component with the same AP length should have a multiple ML widths for anatomical fit. In addition, due to the anthropometric differences of various ethnicities, it is necessary to design and tailor the prostheses with normal anatomical fit for each ethnic group. In this study, we tried to investigate the

anthropometric dimensions of femur to improve the design of the existing prostheses. This data may be useful for designing fully fitted implants with a resected surface of the bone.

**Disclosure:** Authors report no conflict of interest.

Ali Birjandinejad MD<sup>1</sup>

Reza Zandi MD<sup>2</sup>

Elham Karimi MSc<sup>3</sup>

1 Orthopedic Research Center, Shahid Kamyab Hospital, Mashhad University of Medical Sciences, Mashhad, Iran

2 Taleghani Hospital, Shahid Beheshti University of Medical Sciences, Tehran, Iran

3 Department of Biology and Anatomical Sciences, Faculty of Medicine, Shahid Beheshti University of Medical Sciences, Tehran, Iran

## References

1. Lowe CJ, Barker KL, Dewey M, Sackley CM. Effectiveness of physiotherapy exercise after knee arthroplasty for osteoarthritis: systematic review and meta-analysis of randomised controlled trials. *Bmj*. 2007; 335(7624):812.
2. Poitras S, Avouac J, Rossignol M, Avouac B, Cedraschi C, Nordin M, Rousseaux C, Rozenberg S, Savarieau B, Thoumie P, Valat JP. A critical appraisal of guidelines for the management of knee osteoarthritis using Appraisal of Guidelines Research and Evaluation criteria. *Arthritis research & therapy*. 2007; 9(6):R126...
3. Chuang SH, Huang MH, Chen TW, Weng MC, Liu CW, Chen CH. Effect of knee sleeve on static and dynamic balance in patients with knee osteoarthritis. *The Kaohsiung journal of medical sciences*. 2007; 23(8):405-11.
4. Divine JG, Hewett TE. Valgus bracing for degenerative knee osteoarthritis: relieving pain, improving gait, and increasing activity. *The Physician and sportsmedicine*. 2005; 33(2):40-6.
5. Mazzuca SA, Page MC, Meldrum RD, Brandt KD, Petty-Saphon S. Pilot study of the effects of a heat-retaining knee sleeve on joint pain, stiffness, and function in patients with knee osteoarthritis. *Arthritis Care & Research: Official Journal of the American College of Rheumatology*. 2004; 51(5):716-21.
6. Haim A, Rozen N, Dekel S, Halperin N, Wolf A. Control of knee coronal plane moment via modulation of center of pressure: a prospective gait analysis study. *Journal of biomechanics*. 2008; 41(14):3010-6.
7. Goldberg VM, Figgie 3rd HE, Figgie MP. Technical considerations in total knee surgery. *Management of patella problems. The Orthopedic clinics of North America*. 1989; 20(2):189-99.
8. Ranawat CS. The patellofemoral joint in total condylar knee arthroplasty. Pros and cons based on five-to ten-year follow-up observations. *Clinical orthopaedics and related research*. 1986 (205):93-9.
9. Fehring TK, Valadie AL. Knee instability after total knee arthroplasty. *Clinical orthopaedics and related research*. 1994 (299):157-62.
10. Ho WP, Cheng CK, Liao JJ. Morphometrical measurements of resected surface of femurs in Chinese knees: correlation to the sizing of current femoral implants. *The Knee*. 2006; 13(1):12-4.
11. Hitt K, Shurman JR, Greene K, McCarthy J, Moskal J, Hoeman T, Mont MA. Anthropometric measurements of the human knee: correlation to the sizing of current knee arthroplasty systems. *JBJS*. 2003; 85(suppl\_4):115-22.
12. Conley S, Rosenberg A, Crowninshield R. The female knee: anatomic variations. *JAAOS-Journal of the American Academy of Orthopaedic Surgeons*. 2007; 15:S31-6.
13. Poilvache PL, Insall JN, Scuderi GR, Font-Rodriguez DE. Rotational landmarks and sizing of the distal femur in total knee arthroplasty. *Clinical Orthopaedics and Related Research*. 1996; 331:35-46.
14. Chin KR, Dalury DF, Scott RD. Comparative measurement of male and female distal femurs during primary total knee arthroplasty. *J Knee Surg*. 2002; 15:213-7.
15. Campbell WC, Canale ST, Beaty JH. *Campbell's operative orthopaedics*. Philadelphia, PA: Mosby.
16. Biau D, Mullins MM, Judet T, Piriou P. Is anyone too old

- for a total knee replacement?. *Clinical Orthopaedics and Related Research*®. 2006; 448:180-4.
17. Noble PC, Gordon MJ, Weiss JM, Reddix RN, Conditt MA, Mathis KB. Does total knee replacement restore normal knee function? *Clinical Orthopaedics and Related Research*®. 2005; 431:157-65.
  18. Yue B, Varadarajan KM, Ai S, Tang T, Rubash HE, Li G. Differences of knee anthropometry between Chinese and white men and women. *The Journal of arthroplasty*. 2011; 26(1):124-30.
  19. Vaidya SV, Ranawat CS, Aroojis A, Laud NS. Anthropometric measurements to design total knee prostheses for the Indian population. *The Journal of arthroplasty*. 2000; 15(1):79-85.
  20. Cheng FB, Ji XF, Lai Y, Feng JC, Zheng WX, Sun YF, et al. Three dimensional morphometry of the knee to design the total knee arthroplasty for Chinese population. *The Knee*. 2009; 16(5):341-7.
  21. Lim HC, Bae JH, Yoon JY, Kim SJ, Kim JG, Lee JM. Gender differences of the morphology of the distal femur and proximal tibia in a Korean population. *The Knee*. 2013; 20(1):26-30.
  22. Mahfouz MR, Merkl BC, Abdel Fatah EE, Booth Jr R, Argenson JN. Automatic methods for characterization of sexual dimorphism of adult femora: distal femur. *Computer methods in biomechanics and biomedical engineering*. 2007; 10(6):447-56.
  23. Dargel J, Michael JW, Feiser J, Ivo R, Koebke J. Human knee joint anatomy revisited: morphometry in the light of sex-specific total knee arthroplasty. *The Journal of arthroplasty*. 2011; 26(3):346-53.
  24. Yue B, Wang J, Wang Y, Yan M, Zhang J, Zeng Y. How the gender or morphological specific TKA prosthesis improves the component fit in the Chinese population?. *The Journal of arthroplasty*. 2014; 29(1):71-4.
  25. Hussain F, Kadir A, Rafiq M, Zulkifly AH, Sa'at A, Aziz AA, Hossain M, Kamarul T, Syahrom A. Anthropometric measurements of the human distal femur: a study of the adult Malay population. *BioMed research international*. 2013; 2013.
  26. Chaichankul C, Tanavalee A, Itiravivong P. Anthropometric measurements of knee joints in Thai population: correlation to the sizing of current knee prostheses. *The Knee*. 2011; 18(1):5-10.
  27. Moghtadaei M, Moghimi J, Farahini H, Jahansouz A. Morphology of proximal tibia in Iranian population and its correlation with available prostheses. *Medical journal of the Islamic Republic of Iran*. 2015; 29:225.
  28. Merchant AC, Arendt EA, Dye SF, Fredericson M, Grelsamer RP, Leadbetter WB, Post WR, Teitge RA. The female knee: anatomic variations and the female-specific total knee design. *Clinical orthopaedics and related research*. 2008; 466(12):3059-65.
  29. Baker K, Goggins J, Xie H, Szumowski K, LaValley M, Hunter DJ, Felson DT. A randomized crossover trial of a wedged insole for treatment of knee osteoarthritis. *Arthritis & Rheumatism*. 2007; 56(4):1198-203.
  30. Fehring TK, Murphy JA, Hayes TD, Roberts DW, Pomeroy DL, Griffin WL. The Coventry Award Paper: Factors Influencing Wear and Osteolysis in Press-Fit Condylar Modular Total Knee Replacements. *Clinical Orthopaedics and Related Research*®. 2004; 428:40-50.
  31. Himanen AK, Belt E, Nevalainen J, Hämäläinen M, Lehto MU. Survival of the AGC total knee arthroplasty is similar for arthrosis and rheumatoid arthritis: Finnish Arthroplasty Register report on 8 467 operations carried out between 1985 and 1999. *Acta orthopaedica*. 2005; 76(1):85-8.
  32. Rand JA, Ilstrup DM. Survivorship analysis of total knee arthroplasty. Cumulative rates of survival of 9200 total knee arthroplasties. *The Journal of bone and joint surgery. American volume*. 1991; 73(3):397-409.
  33. Rand JA, Trousdale RT, Ilstrup DM, Harmsen WS. Factors affecting the durability of primary total knee prostheses. *JBJS*. 2003; 85(2):259-65.
  34. Robertsson O, Knutson K, Lewold S, Lidgren L. The Swedish Knee Arthroplasty Register 1975-1997: an update with special emphasis on 41,223 knees operated on in 1988-1997. *Acta Orthopaedica Scandinavica*. 2001; 72(5):503-13.
  35. Booth RE. The gender-specific (female) knee. *Orthopedics*. 2006; 29(9):768-9.
  36. Barrett WP. The need for gender-specific prostheses in TKA: does size make a difference?. *Orthopedics*. 2006; 29(9):S53.
  37. Dorr LD, Boiardo RA. Technical considerations in total knee arthroplasty. *Clinical orthopaedics and related research*. 1986 (205):5-11.